
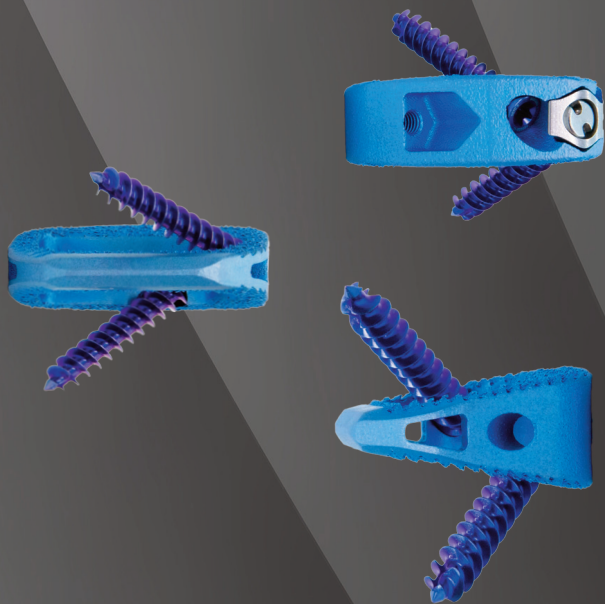


ALIGN AO

ANTERIOR LUMBAR SYSTEM
FOR OBLIQUE APPROACH

The Align AO is a spinal system that is **implanted in the intervertebral body space via an anterior approach to improve the stability of the spine while supporting fusion**. Components are offered in different shapes and sizes to meet the requirements of the individual patient's anatomy. Made from additively manufactured titanium alloy (Ti-6Al-4V ELI).

The Align AO provides an effective **anterolateral approach to maximize options available to the surgeon when an alternative to a true anterior approach is required**. The design and porous structure improves adhesion to vertebral body endplates to support bone in-growth when used with allogenic bone graft and/or autograft to facilitate fusion.

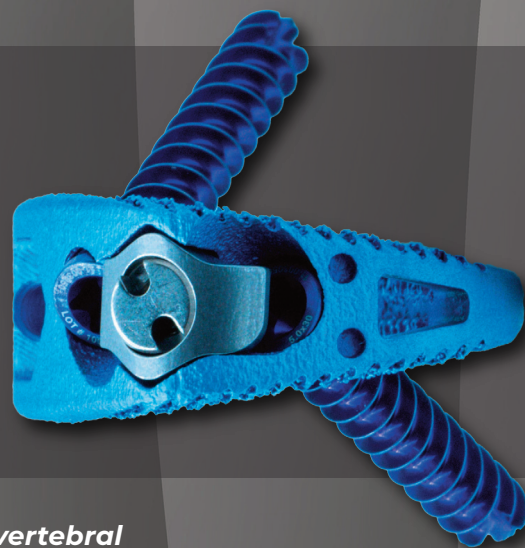

DUAL ANTEROLATERAL INSERTION FEATURES

Maximizes ability to place anterolateral implant across midline or directly anterolateral.

ENHANCED POROUS STRUCTURE

Increases bone in-growth to endplate

SIMPLE INSTRUMENTATION

Enhances surgeon efficiency with comfortable handles

ALIGN AO




ANTERIOR LUMBAR SYSTEM
FOR OBLIQUE APPROACH

INDICATIONS FOR USE

The Align AO system is **indicated for intervertebral body fusion of the spine in skeletally mature patients who have had at least six months of non-operative treatment.** The device systems are designed for use with allogenic bone graft comprised of cancellous and/or corticocancellous bone graft allograft and/or autograft to facilitate fusion. One device is used per intervertebral body space.

The Align AO system is **intended for use at either one level or two contiguous levels in the lumbar spine, from L2 to S1, for the treatment of degenerative disc disease (DDD) with up to Grade I spondylolisthesis.** DDD is defined as back pain of discogenic origin with degeneration of the disc confirmed by history and radiographic studies.

The Align AO system intended to be used with a supplemental spinal fixation system **cleared for use in the lumbosacral spine.**

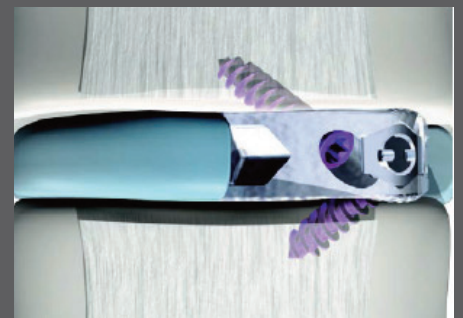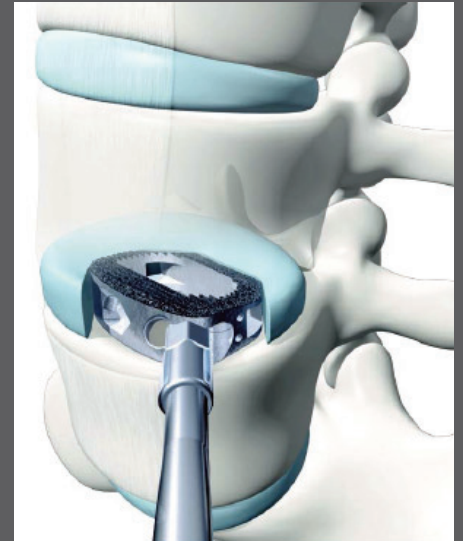

Footprints

XS	32 x 21
S	32 x 24
L	36 x 26
XL	38 x 30

All footprints available in 2-screw configurations

UNITARY TITANIUM STANDARD SIZES

Lordosis	Height
25°	- - - - - 15 16 17 18 19 20 21 22
20°	- - - - - 15 16 17 18 19 20 21 22
16°	- 11 12 13 14 15 16 17 18 19 20 21 22
12°	10 11 12 13 14 15 16 17 18 19 20 21 22
7°	10 11 12 13 14 15 16 17 18 19 20 21 22



Align AO Surgical Technique Guide
is available upon request

844.228.4890 • support@AcuitySurgical.com • AcuitySurgical.com

LBL-AS202602 Rev A.01